


# Z2 TENSION RANGES

## Sample Dial Faces

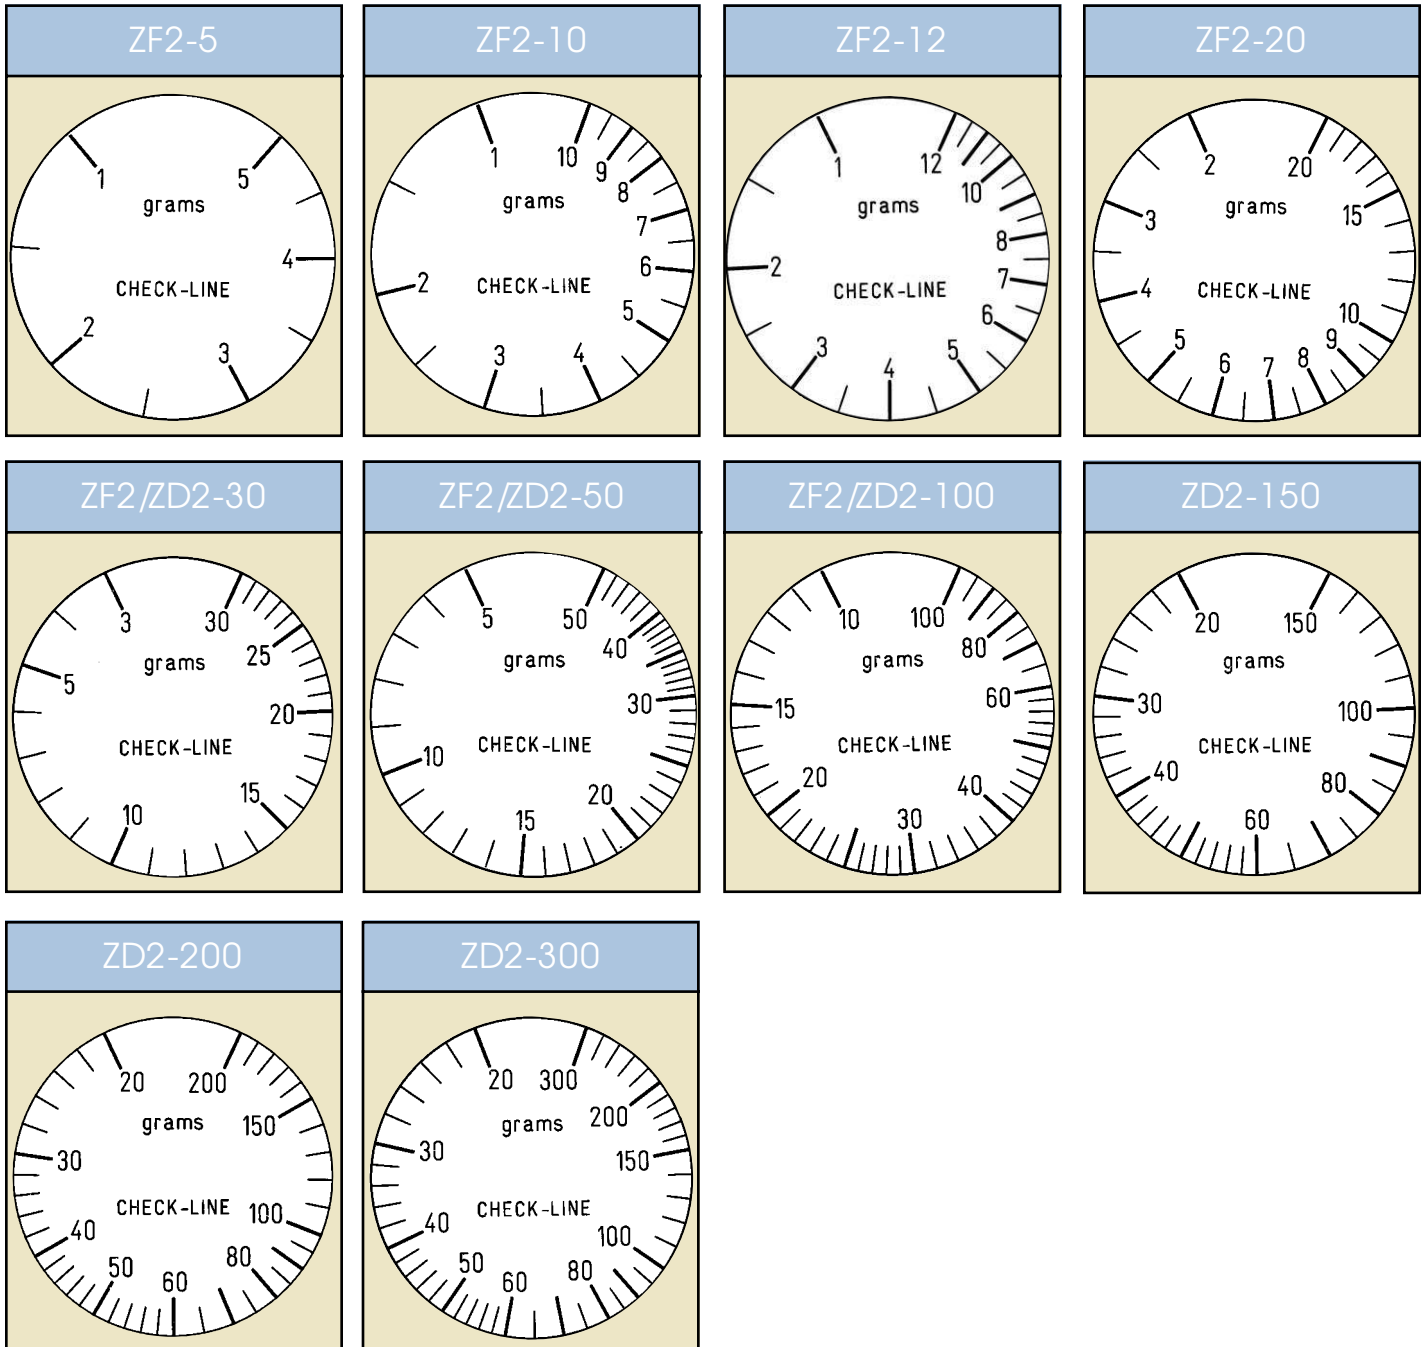

### NOTES

1. The dial face marking of each instrument can differ slightly from the samples above since each instrument is calibrated and marked by hand to optimize accuracy.
2. Dial faces shown above are reduced 20% from actual size.