

PosiTector[®] **SPG**

Surface Profile Gage

Quick Guide v. 1.0





Introduction

The **PosiTector Surface Profile Gage (SPG)** is a hand-held electronic instrument that measures the peak-to-valley height of the surface profile of abrasive blast cleaned surfaces. It consists of a body (Standard or Advanced) and probe.

This Quick Guide summarizes the basic functions of the instrument. Download the full instruction manual at: www.defelsko.com/manuals

Quick Start

The **PosiTector SPG** powers-up when the center navigation button  is pressed. To preserve battery life, the instrument powers down after approximately 5 minutes of no activity. All settings are retained.

1. Remove the protective plastic cap from probe.
2. Power-up Gage by pressing the center navigation  button.
3. Place the glass plate onto a stable, flat surface. Take several measurements. If the average is greater than $\pm 5 \mu\text{m}$ (0.2 mil), zero the instrument (see pg. 4).
4. Place the probe FLAT on the surface to be measured such that the tip of the probe reaches into the bottom of a profile valley. HOLD STEADY. The Gage will BEEP twice and display the measurement.
5. Lift the probe from the surface between measurements.

Probe

To disconnect a probe from a body, power-down the instrument and slide the plastic probe connector horizontally (in the direction of the arrow) away from the body. Reverse these steps to attach a new probe.



When powered-up, the **PosiTector** automatically determines which type of probe is attached and does a self-check.

The supplied probe tip has a 60° angle to comply with most test standards including ASTM D 4417 B. An optional 30° angle tip with replacement tool is available for special applications or to comply with Australian Standard AS 3894.5.

Calibration

Instrument calibration is typically done by the manufacturer or qualified lab. All probes include a Certificate of Calibration.

Verification of Accuracy

Instrument accuracy is verified using the included metal shim and glass zero plate. Ensure that the glass plate and shim are clean and dirt free before use.

Place the plate onto a stable, flat surface. Take several measurements. If the average is greater than $\pm 5 \mu\text{m}$ (0.2 mil), zero the instrument (see below).


Next, place the metal shim over the glass plate and measure ensuring the probe needle touches the glass plate in the area between the shim's "legs". The average of several measurements should be within the combined tolerances of both the gage and the shim. If not, see Returning for Service (pg. 8). Metric example: gage tolerance is $\pm 5\%$ or $\pm 5 \mu\text{m}$ whichever is greater. The 76 μm shim tolerance is $\pm 5 \mu\text{m}$. So the average of several measurements should be between 66 and 86 microns. Inch example: gage tolerance is $\pm 5\%$ or ± 0.2 mils whichever is greater. The 3 mil shim tolerance is ± 0.2 mils. So the average of several measurements should be between 2.6 and 3.4 mils.

Zeroing the Instrument

The **PosiTector SPG** has only one adjustment point at zero. The zero point can be set using one of two methods. Both methods are found under the Zero menu option.




Glass Plate Zero

Setting the instrument to zero on the glass plate is the preferred zero adjustment method:

1. Select  from the menu.
2. Press the (+) button to select the number of readings to be used to obtain an average, typically 3.
3. Repeatedly measure the glass plate. After the last measurement, the gage will calculate a Zero which represents the average of all the Zero readings taken.

Factory Zero

If a glass plate or suitable smooth, hard surface is not available, the factory zero setting can be restored:

1. Select  from the menu.
2. Press the down button to select “Reset” and press the center navigation button.  The factory calibration icon  will appear on the LCD.

NOTE: -The factory zero setting may not always be precise, particularly after a probe tip exchange. For best accuracy, the gage should be zeroed on the included glass plate.

Setup Menu

 **Reset**

Reset (soft reset) restores factory settings and returns the instrument to a known condition. The following occurs:



- All batches, stored measurements, images, and batch names are erased.
- The zero adjustment is returned to the factory setting. Since this may not always be a precise zero, the gage should be checked on the glass plate.
- Menu settings are returned to the following:

Memory = OFF

Statistics Mode = OFF

Hi Lo Alarm = OFF

Bluetooth = OFF

Perform a more thorough **Hard Reset** by powering down the instrument, waiting several seconds, then simultaneously holding both the center  and **(+)** buttons until the **Reset** symbol  appears. This returns the instrument to a known, “out-of-the-box” condition. It performs the same function as a menu **Reset** with addition of:

- Bluetooth Pairing info is cleared.
- Menu settings are returned to the following:

Units = microns	Language = English
Flip Display = Normal	Battery Type = Alkaline
Auto Sync = OFF	Backlight = Normal
White on Black = OFF	Bluetooth Streaming = OFF
USB Drive = ON	

NOTES: - Date and Time are not affected by either **Reset**.

Battery Type

Selects the type of batteries used in the instrument from a choice of “Alkaline”, “Lithium” or “NiMH” (Nickel-metal hydride rechargeable). If NiMH is selected, the instrument will trickle charge the batteries while connected via USB to a PC or optional AC charger. The battery state indicator icon is calibrated for the selected battery type. No damage will occur if the wrong battery type is selected.

NOTE: DeFelsko recommends the use of *eneloop* (NiMH) rechargeable batteries.

Statistics Menu

Statistics

 \bar{x}

A statistical summary will appear on the display. Remove the last measurement by pressing the **(-)** button. Press **(+)** to clear statistics.

\bar{x} - Average

σ - Standard Deviation

\uparrow - Maximum Value

\downarrow - Minimum Value

HiLo Alarm

Allows the Gage to visibly and audibly alert the user when measurements exceed user-specified limits.


Memory Management

The **PosiTector SPG** can record readings in memory for printing to the optional Bluetooth wireless printer, transfer to a computer (pg. 6) or synchronizing with *PosiTector.net*. Readings are time-stamped as they are taken.

Scroll through display modes
(*Advanced only*)

Delete last reading


Access the Menu

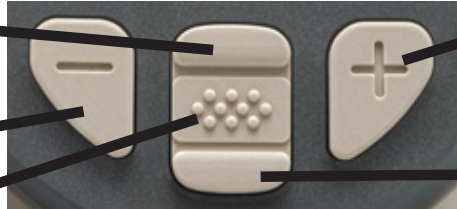

Create a new batch
(*Advanced only*)

Restore brightness
after dimming
(*Advanced only*)

Standard models store up to 250 readings in one batch.

Advanced models store 100,000 readings in up to 1,000 batches. “New Batch” closes any currently opened batch and creates a new batch name using the lowest available number. The  icon appears. New batch names are date stamped when they are created.

SmartBatch™

This menu option sets-up the **PosiTector SPG** to comply with various standards and test methods published by organizations including ASTM, SSPC, ISO, IMO, US Navy, SANS and AS.

For instructions on how to use the Smart Batch™ feature, see www.defelsko.com/smartbatch

Outputting Stored Readings

USB mass storage - connect your **PosiTector** to a PC/Mac using the supplied USB cable to access and print stored readings and graphs. No software or internet connection required.

PosiTector.net - a free web-based application offering secure centralized storage of thickness readings. Access your readings from any web connected device. www.PosiTector.net

Connect Menu

Sync Now

Immediately initiates synchronization with *PosiTector.net* when connected (USB or Bluetooth) to an internet connected PC running *PosiTector Desktop Manager*.

Auto SYNC



Allows the instrument to automatically synchronize with *PosiTector.net* when initially connected to an internet connected PC running *PosiTector Desktop Manager*.

Additional measurements added to memory while connected are synchronized only when the USB cable is disconnected, then reconnected or when **Connect > Sync Now** is selected.

USB Drive



The instrument uses a USB mass storage device class which provides a simple interface to retrieve data in a manner similar to USB flash drives, cameras or digital audio players.

NOTE: When connected, power is supplied through the USB cable. The batteries are not used and the body will not automatically power down. If rechargeable (NiMH) batteries are installed, the instrument will trickle charge the batteries.

Bluetooth

(Advanced models only)



Allows individual readings to be sent to a computer or compatible device as they are taken using Bluetooth wireless technology. See www.defelsko.com/bluetooth

Updates

Determines if a software update is available for your instrument. Must be connected to an internet connected PC running *PosiTector Desktop Manager*. See www.defelsko.com/update

NOTE: The instrument may perform a **Hard Reset** (pg. 4) after updating.

Returning for Service

Before returning the instrument for service...

1. Install new or newly recharged batteries in the proper alignment as shown within battery compartment.
2. Examine the probe tip for dirt or damage. The probe tip should move up and down freely. The metal plate surrounding the probe tip should be smooth and free from burrs and foreign material.
3. Perform a **Hard Reset** (pg. 4).
4. Place the metal shim over the glass plate and attempt a measurement.

If you must return the instrument for service, please fill out and include the service form located at www.defelsko.com/support with the instrument.