



Factory Certificate of Calibration

Product Name	LOGIC BASIC	Name of Inspection Standard	Ig2110
Model No.		Unit	inch
Serial No.		Scale Interval	0.0001 inch
Certificate No.		Measuring Range	1 inch
		Reference Point	0 inch
		End Point	1 inch

N.I.S.T. No. 821/268795-03

Inspection Item Name	Result	Permissible Value	Judgment
Indication Error	0.0000611 inch	0.0002 inch	GO
Hysteresis	-----	0.0001 inch	N/A
Repeatability	0.000002 inch	0.0001 inch	GO
Max. Measuring Force	-----	-----	N/A

Inspection Item Name	Judgment
Inspection of Function and Appearance	GO

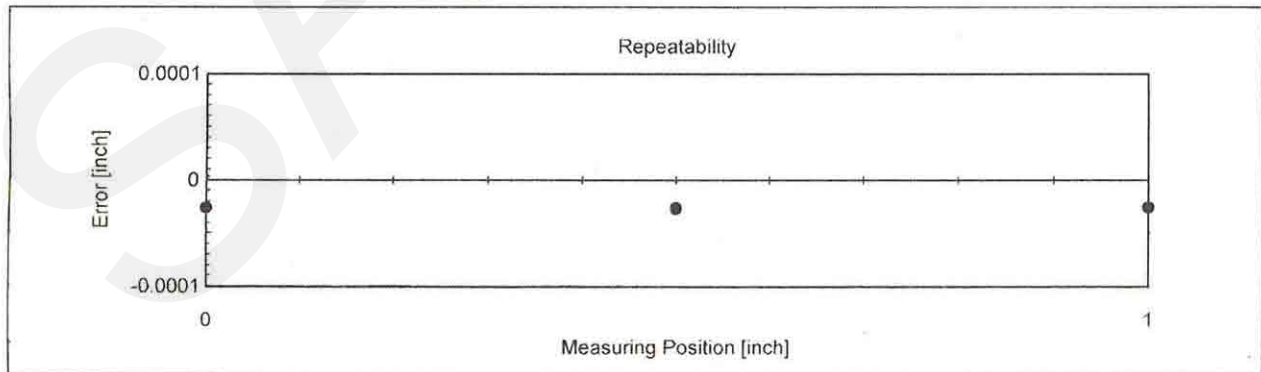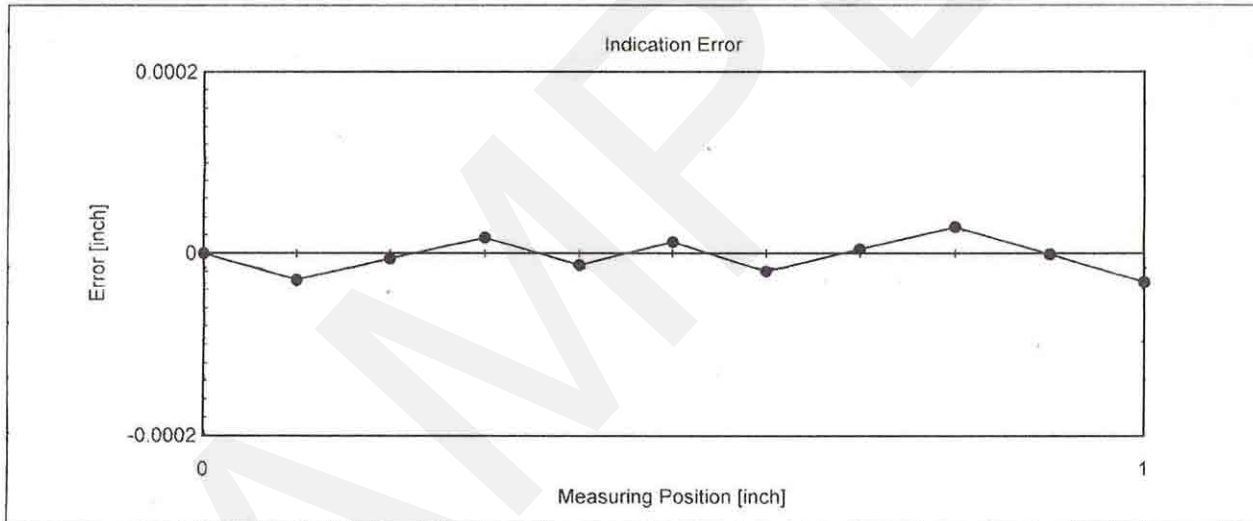

Signature: _____

Visit us on the World Wide Web at www.checkline.com

ELECTROMATIC Equipment Co., Inc., 600 Oakland Ave., Cedarhurst, NY 11516 – USA
 Tel: 800-645-4330 (USA & Canada) ■ Tel: (516) 295-4300 ■ Fax: (516) 295-4399